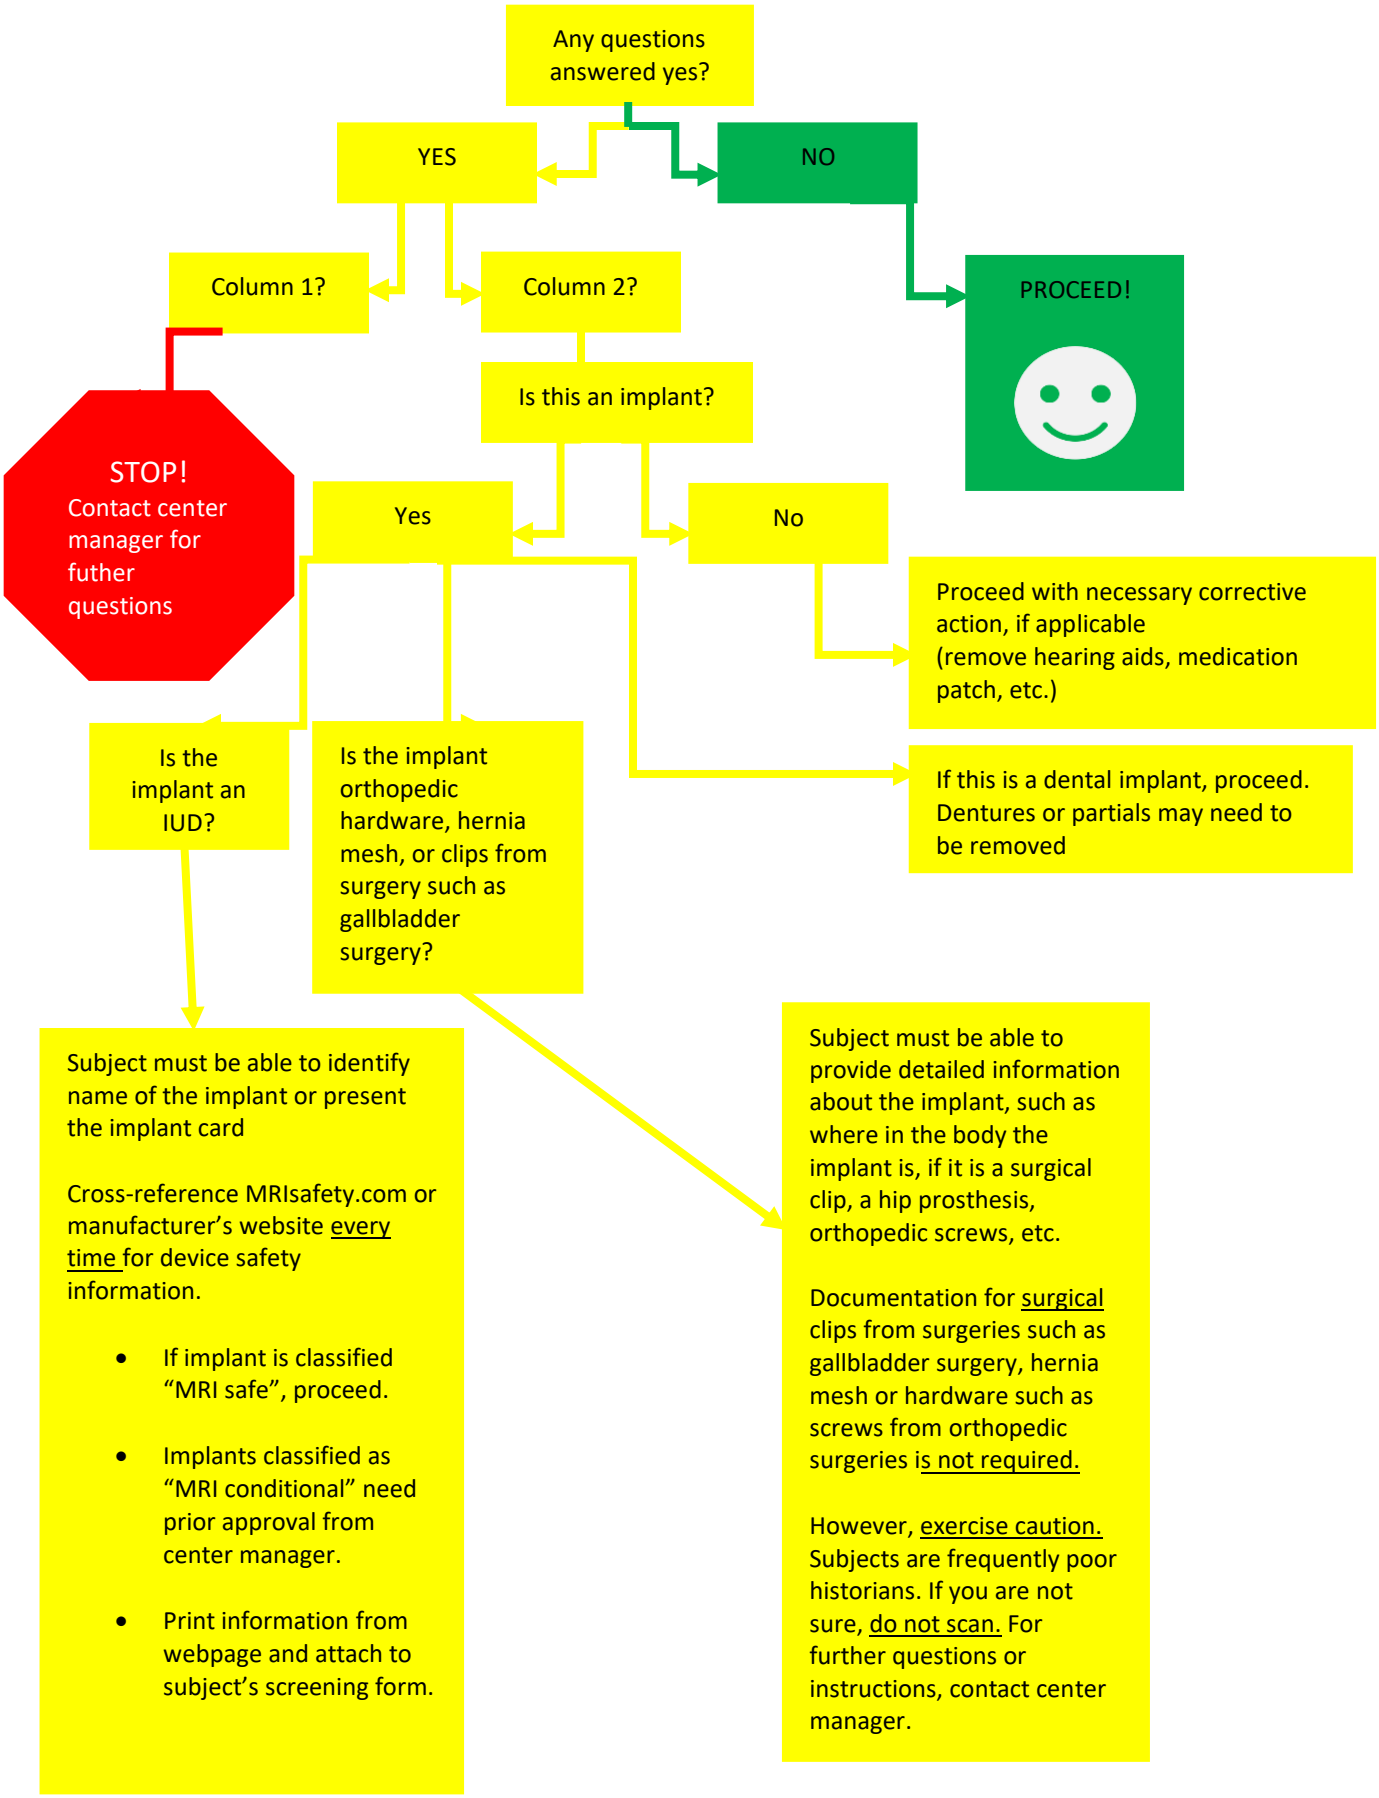
Any questions answered yes?
YES
NO
PROCEED!
Column 1?
Column 2?
STOP!
Contact center manager for futher questions
Is this an implant?
Yes
No
Proceed with necessary corrective action, if applicable (remove hearing aids, medication patch, etc.)
Is the implant an IUD?
Is the implant orthopedic hardware, hernia mesh, or clips from surgery such as gallbladder surgery?
If this is a dental implant, proceed. Dentures or partials may need to be removed
Subject must be able to identify name of the implant or present the implant card
Cross-reference MRIsafety.com or manufacturer's website every time for device safety information.
• If implant is classified "MRI safe", proceed.
• Implants classified as "MRI conditional" need prior approval from center manager.
• Print information from webpage and attach to subject's screening form.
Subject must be able to provide detailed information about the implant, such as where in the body the implant is, if it is a surgical clip, a hip prosthesis, orthopedic screws, etc.
Documentation for surgical clips from surgeries such as gallbladder surgery, hernia mesh or hardware such as screws from orthopedic surgeries is not required.
However, exercise caution. Subjects are frequently poor historians. If you are not sure, do not scan. For further questions or instructions, contact center manager.